



FDR nano

Designing a new workflow

How often do you encounter the problem with mobile X-ray in a daily medical situation?

FUJIFILM Provides a New Solution with Compact Digital X-ray Cart system for Critical Moments you face everyday.



Amazing future
with "nano"

Patient friendly

Minimum exposure is desirable when taking X-ray images of a new born or infant. Dramatic dose reduction is possible by utilizing FUJIFILM core technology.



Ultra-high sensitivity system

DR Cassette FDR D-EVO II

- High sensitivity reading technology "ISS"
- Noise reduction circuit (NRC) on board




Image processing technology Virtual Grid (VG)

- Provides a high-contrast image without using a grid
- Improves image granularity in low-dose imaging



Virtual Grid

Proprietary technology has achieved a significant dose reduction

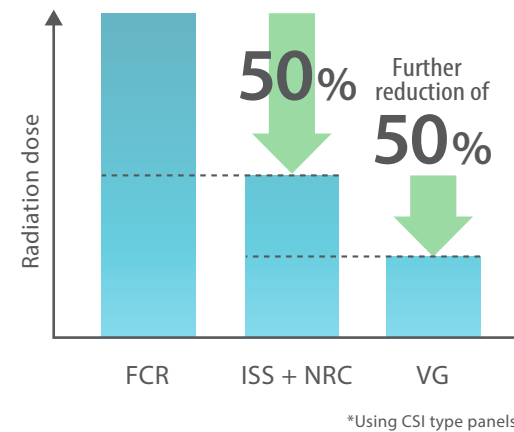

Small X-ray tube dedicated to the ultra-high sensitivity system



Quiet

Stationary anode X-ray tube does not make noise to surprise the patient

Slim

Easily position the tube head over the incubators


Quick accessibility

Medical scene such as Emergency rooms are crowded with equipments and staffs. Freedom of movement is possible with four wheel caster and extremely light weight X-ray cart.




Small size and lightweight

Traditional mobile X-ray

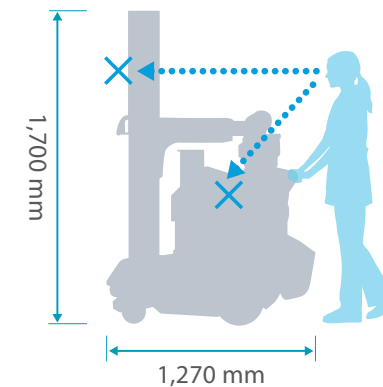

Total weight	500kg	X-ray tube part	20kg
--------------	-------	-----------------	------

FDR nano

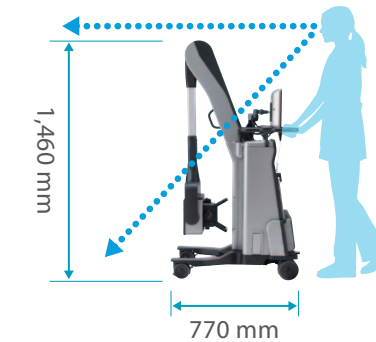


Total weight	90kg	X-ray tube part	10kg
--------------	------	-----------------	------



Unlimited movement

Spin & slide

Four wheel caster enables superb movement control at ones will.

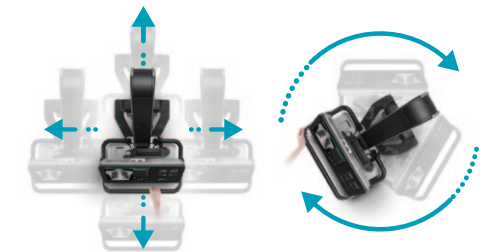

■ Little downtime



High performance Li-ion battery enables quick charge of 4 hours and can be used continuously for 12 hours. Also plugged in exposure is possible.

■ Ready to be used at anytime



D-EVO II is charged when placed in the DR slot and is quickly taken out with tilting function.

■ Quick viewing while treating



Operation panel can rotate freely according to the doctor's position.

Innovation to the Workflow

Combining FUJIFILM core technology of Cassette DR with image processing and compact Digital X-ray cart, we provide a innovation to the workflow of taking X-rays.



FDR D-EVO II
Cassette DR suitable for mobile exposure

- Easy to insert between patients and bed.
- Light weight panels make easy handling.

FDR nano

SMW (Smart Mobile Workflow)

Digital X-ray cart

- Reduce weight by 1/5 compared to conventional x-ray mobile, providing easy handling.

Virtual Grid

Virtually created grid

- Provide a flexible exam without a physical Grid exam.
- Over come situation where physical grid can be challenging or disruptive to patient comfort.

Approx. 2.6 kg

*D-EVO II C35.

Virtual Grid 0 kg (Software)

Real Grid Approx. 1 kg

Example of image unevenness Caused by a grid misalignment

Pinpoint movement

Even in narrow spaces such as bedside and elevator, changing direction can be done with ease.

Easy positioning

Simply sliding or turning the whole apparatus enables easy position changes.

The shortest moving distance

The slim body allows technologists to make minimum moves in device operation and positioning.

Maintaining Clean Equipments

Medical equipment surface tends to have high risk for transferring germs, and it is essential to maintaining clean equipments in Operation rooms.



D-EVO II, and some parts of the FDR nano*, we have applied our antibacterial technology "Hydro Ag".

*Shot Switch, surface of Operation Panel

Easy to clean with flat surface

IPX6 waterproofing cassette DR

Easy bagging

Easy to clean with cordless surface

Antibacterial coating

As for the Hydro Ag it has high anti bacterial performance preventing germs from growing. This is 100 times more effective than conventional coating, and 10,000 times more protection than surface with no coating.

Conventional

Hydro Ag

JIS Z 2801/ISO 22196 complied test (Escherichia coil)

Number of residual bacterial after one hour


Coating	Residual bacterial count (cps/cm2) after one hour
Without coating	~100,000
Poor-hydrophobic binder coating (Conventional)	~1,000
Hydro Ag coating	~10

Tested by BOKEN Quality Evaluation Institute
Report ID: 20214016660-1(Jul 11, 2014)

Specifications



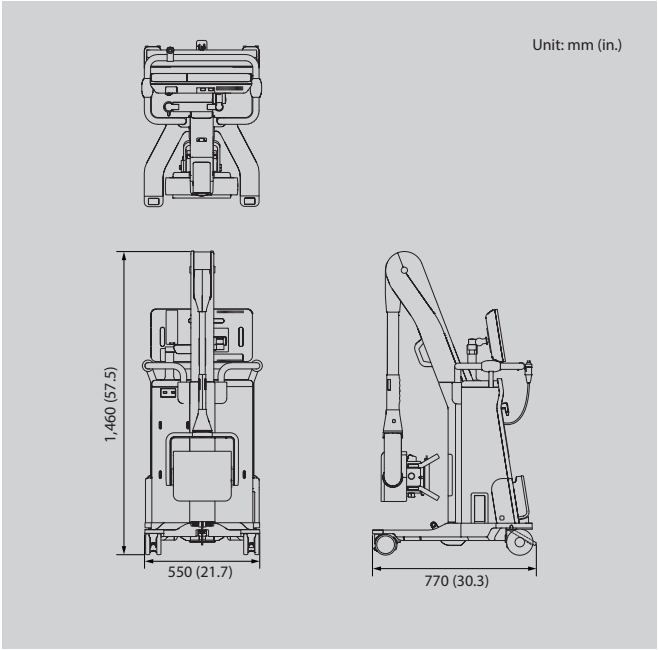


Product name	FDR nano
Model No.	DR-XD1000
Power supply	100-240 V AC, Single phase: 50-60 Hz 8-3.3 A
X-ray output	Max. rating: 2.5 kW Tube voltage: 40-100 kV Tube current: Max 35 mA
X-ray tube	Nominal focal spot size 1.2 mm maximum anode heat capacity 35 kJ (50 kHU) Target angle: 16 degree
Total width	550 mm (excluding handle fix part)
Total length	770 mm
Total height	1,460 mm
Weight	90 kg



Optional Items

- High handle kit
- Added filter
- Accessory case
- Apron hanger
- BCR
- Wet tissue holder
- DAP meter fix kit

System Components : Flat Panel Sensor

	D-EVOII C24	D-EVOII C35	D-EVOII C43
			
Scintillator	CsI (Cesium iodide)	CsI (Cesium iodide)	CsI (Cesium iodide)
Detector external size	328 × 268 × 15 mm (Approx.) [12.9" × 10.6" × 0.6"]	460 × 384 × 15 mm (Approx.) [18" × 15" × 0.6"]	460 × 460 × 15 mm (Approx.) [18" × 18" × 0.6"]
Weight	Approx. 1.5 kg [3.3 lbs.] (including battery)	Approx. 2.6 kg [5.7 lbs.] (including battery)	Approx. 3.2 kg [7.1 lbs.] (including battery)

•Specifications are subject to change without notice. •All brand names or trademarks are the property of their respective owners.
•All products require the regulatory approval of the importing country. •For details on their availability, contact our local representative.

FUJIFILM

FUJIFILM Corporation
26-30, NISHIAZABU 2-CHOME, MINATO-KU, TOKYO 106-8620, JAPAN
<http://www.fujifilm.com/products/medical/>

Ref. No. XB-1043E (SK-16-12-F1079-F8598) Printed in Japan ©2016 FUJIFILM Corporation

FUJIFILM
Value from Innovation



FDR nano

Designing a new workflow